FloSpine

CANAVERAL

PEDICLE SCREW SYSTEM

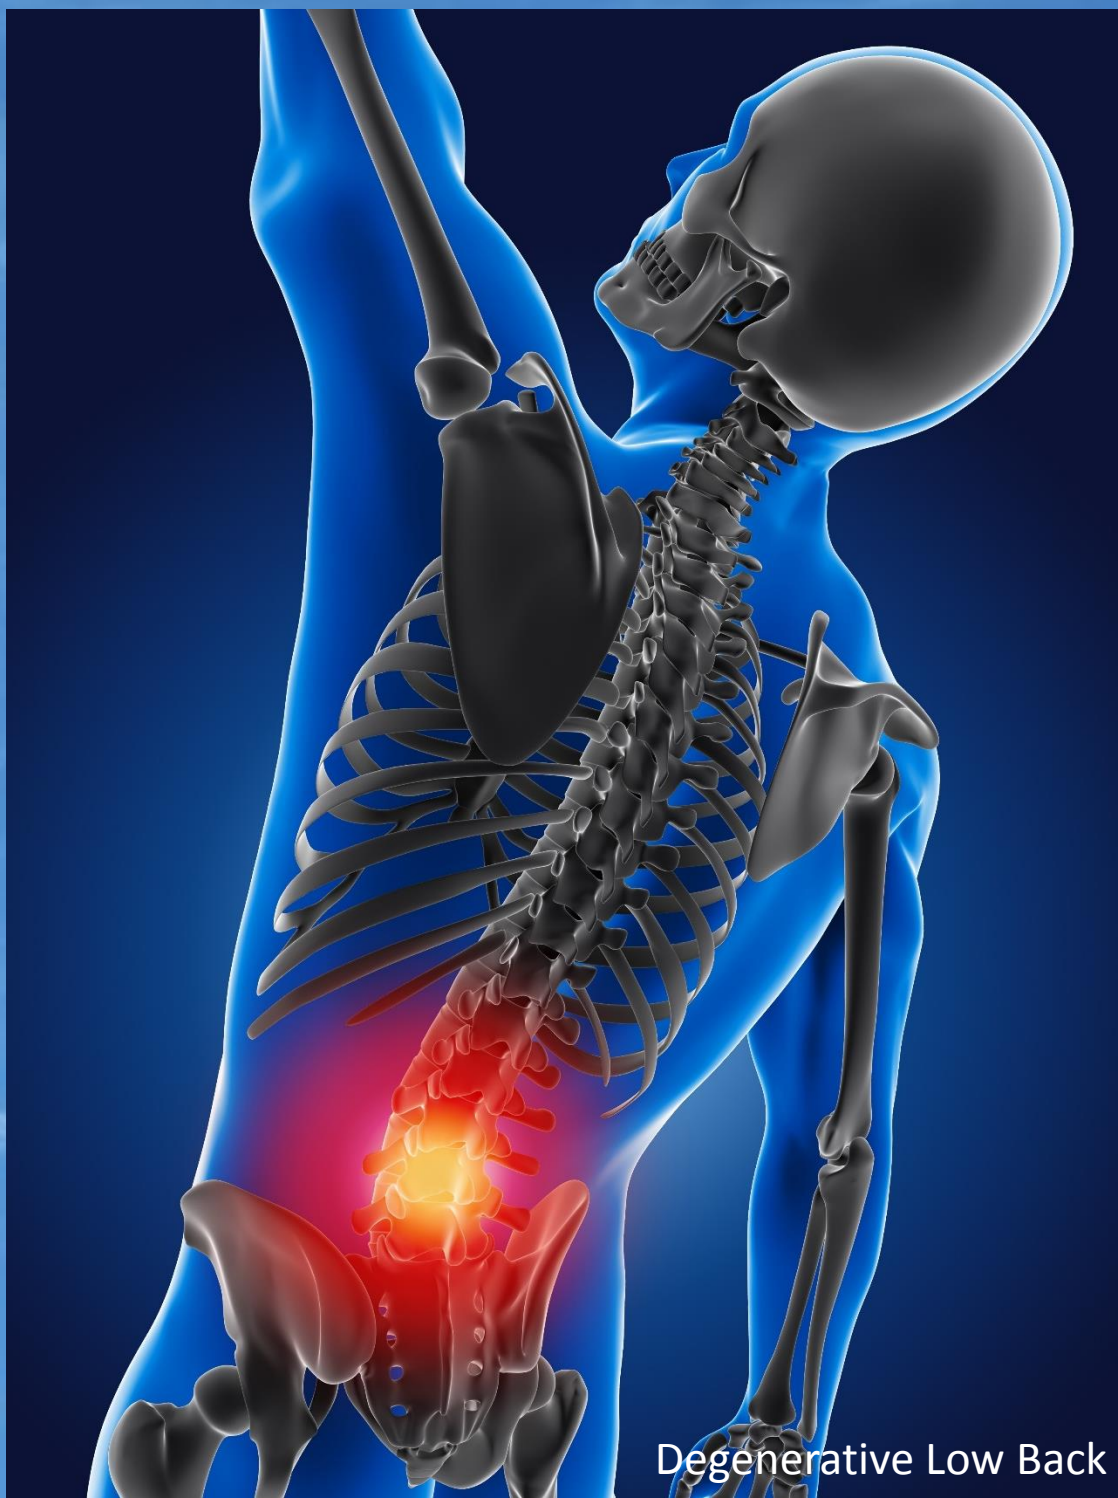

We've Got
Your Back™

Degenerative Low Back

CANAVERAL
PEDICLE SCREW SYSTEM

DESIGN MAKES

PRECISION IMPLANTS

- ✓ **Low profile headbody**
- ✓ **Accepts 5.5mm & 6.0mm Diameter rods, Ti & CoCr, Straight and Pre-lordosed**
- ✓ **Friction Style Headbody**
- ✓ **Pre-Assembled and Modular Options**
- ✓ **EASYSTART™ Anti-Cross-threading Set Screw Facilitates Introduction**
- ✓ **Self-Tapping, Duel Lead, Optimized Thread form for fast delivery and pull out resistance**
- ✓ **60° full conical motion provides exceptional anatomic adjustability**
- ✓ **Comprehensive Screw Offering, 4.5mm-10.5mm**

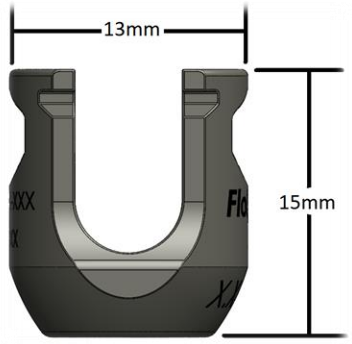

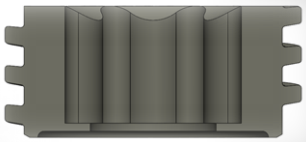

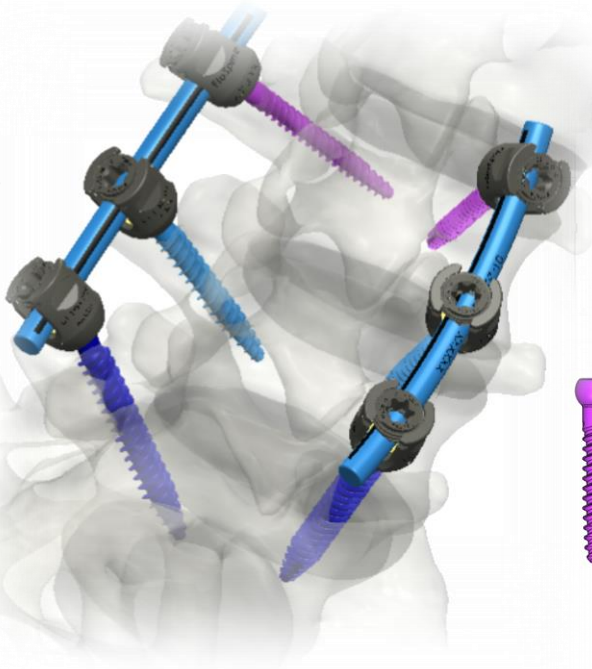

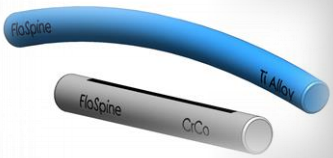

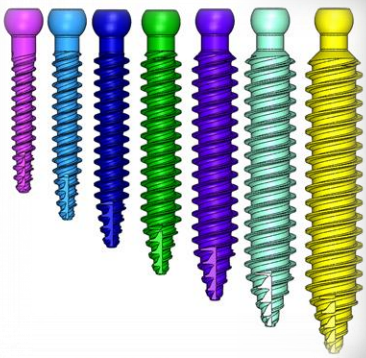

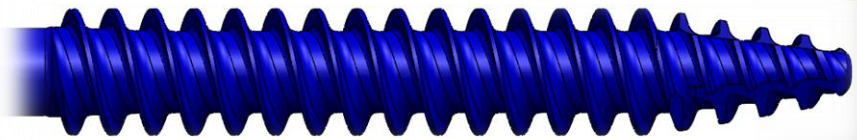

		Screw Length (mm)												
		25	30	35	40	45	50	55	60	70	80	90	100	110
Screw Diameter (mm)	4.5	*	*	*	*	*								
	5.5	*	*	*	*	*	*	*						
	6.5	*	*	*	*	*	*	*	*					
	7.5		*	*	*	*	*	*	*					
	8.5			*	*	*	*	*	*	*	*	*	*	*
	9.5			*	*	*	*	*	*	*	*	*	*	*
	10.5				*	*	*	*	*	*	*	*	*	*

THE DIFFERENCE

INTUITIVE INSTRUMENTATION

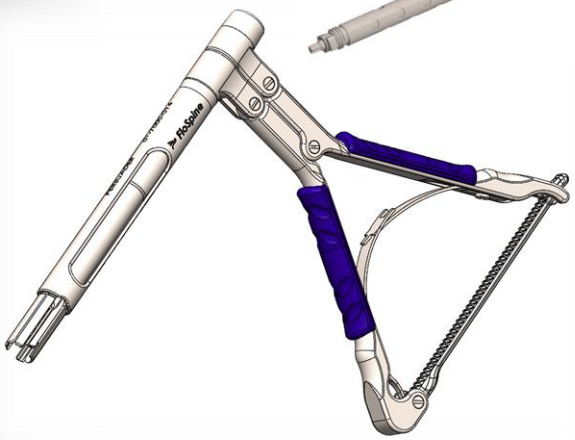

- ✓ **Quick connect Pistol Grip, Threaded, and Rod Rocker reduction / manipulation**
- ✓ **Elite Locking Screw Drivers**
- ✓ **Screw Inserter and Headbody delivery instruments for in-situ assembly**
- ✓ **Color coded taps match screw diameters for fast screw prep**
- ✓ **Adapted for use with surgical navigation systems**
- ✓ **Multiple handle options to meet a variety of surgeon preferences**
- ✓ **Chrome coated instruments extend instrument life and quality**
- ✓ **Sterilization Cases follow surgical procedure**

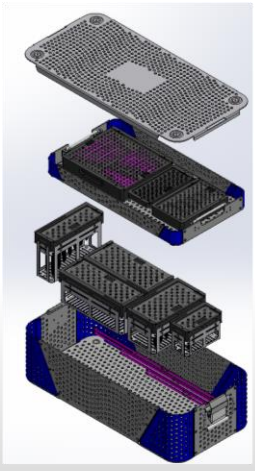

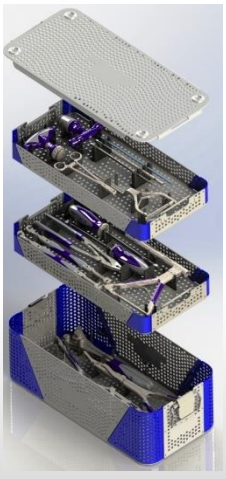

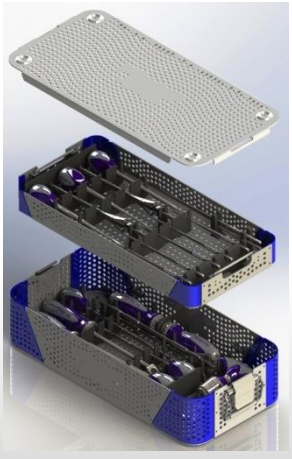

FloSpine

INDICATIONS

The FloSpine Canaveral Pedicle System is intended for posterior, noncervical pedicle fixation as an adjunct to fusion in skeletally mature patients using autograft and/or allograft for the following indications: degenerative disc disease (DDD) (defined as back pain of discogenic origin with degeneration of the disc confirmed by history and radiographic studies); spondylolisthesis; trauma (i.e., fracture or dislocation); spinal stenosis; curvatures (i.e., scoliosis, kyphosis, and/or lordosis); tumor; pseudoarthrosis; and failed previous fusion.

When used for fixation to the ilium, the offset connectors of the Canaveral Pedicle Screw System must be used in conjunction with pedicle screws placed at the S1 or S2 spinal levels.
When used for posterior non-cervical pedicle screw fixation in pediatric patients, the Canaveral Pedicle Screw System implants are indicated as an adjunct to fusion to treat adolescent idiopathic scoliosis. The Canaveral Pedicle Screw System for pediatric use is intended to be used with autograft and/or allograft. Pediatric pedicle screw fixation is limited to the posterior approach.

Manufactured in United States of America
* Other sizes not shown available upon request
Caution: Federal law (USA) restricts this device to sale by or on the order of a physician
561-705-3080
www.flospine.com
XR-1309-PL-US FloSpine, LCC 11/2014

FloSpine, LLC
Boca Raton, Florida
561-705-3080
www.flospine.com